

Real Rife

Real Rife therapy - producing the same treatment output as the original machines used by Dr Royal Raymond Rife himself



Not all Rife machines are created equally. The Real Rife Therapy System has been developed with a team of researchers and engineers over the course of 10 years, with the aim of understanding and reproducing as far as possible the technology used by Rife in his own machines.

DESIGNED TO DELIVER RESULTS

Not all Rife machines are created equally. Most "Rife" resonators do not produce the correct output that was developed by Dr Rife, something that can easily be demonstrated by means of a spectrum analyser and oscilloscope.

Rife was the only one whose technology got the amazing results that everyone thinks of when they hear the name Rife. It therefore follows that until we know more than Rife (which we clearly don't!) we should be doing things exactly the way he did (as far as is possible) if we hope to get similar results. Furthermore, Rife was very clear that things had to be done very specifically and very accurately or the technology simply would not work!



Based on the data obtained from an original Rife machine, using a spectrum analyser and oscilloscope, the Real Rife Therapy System was successfully developed to produce the same frequencies, wave forms and relative power as Rife's original machines.

There are many Rife machines available these days, but it is crucial to make sure that you are buying a Rife machine that can measure up to Rife's original technology. The shortcoming of other "Rife" machines is that they simply do not produce the same wave forms, frequencies and relative power as Rife's original machines, and therefore do not produce the same results. The Real Rife system has been tested and shown (measured with a spectrum analyser and oscilloscope) to create the same Hoyland wave forms, frequencies and relative power as specified by Rife. Without measuring the output with a spectrum analyser and oscilloscope, it is impossible to know what a Rife machine is producing and how it compares to Rife's specifications.

THE REAL RIFE THERAPY SYSTEM GUARANTEES:

THE CORRECT FREQUENCIES

- Frequency sweep from 2Mhz–5Mhz (measured on spectrum analyser).

THE CORRECT WAVE SHAPE

- An actual Hoyland wave form (measured on oscilloscope).

THE CORRECT RELATIVE POWER

- At least 1W on contact (measured on oscilloscope).

Ensure that you are getting a Rife machine that will produce results by asking if the machine's output can be demonstrably measured by spectrum analyser and oscilloscope to comply with Rife's specifications. The Real Rife Therapy System ticks all the boxes needed to ensure therapeutic efficacy.

TRUE TO RIFE'S OWN SPECIFICATIONS

The Real Rife Therapy System can demonstrably produce the frequencies, wave shape, and relative power specified by Dr Rife. These measurements can be made with a spectrum analyser and oscilloscope and are crucial in showing that the Rife machine is up to the standard required for therapeutic results.

FREQUENCIES:

The original frequencies recorded and used by Dr Rife are not estimated values, but values that have been determined by studying all the known Rife documents and measuring the actual output of three original Rife machines. The spectrum analyser pattern should show the central high frequency carrier wave, with multiple side-band frequencies generated simultaneously. The frequency range should be between 2Mhz and 4Mhz, with a frequency sweep from 2Mhz–5Mhz to target all pathogens.

WAVE SHAPE :



The wave shape produced by Rife's machines is the Hoyland wave, which is an interrupted (aka gated) wave resembling a modulated square wave. Many "Rife" machines produce a square wave instead of a proper Hoyland wave. The Hoyland wave form is not a square wave, but rather a wave that is produced using a sine wave audio frequency modulated onto a sine wave RF carrier frequency.

RELATIVE POWER:

A minimum power level of 1W with at least 70V is required to penetrate the most resistive tissues when the hand contact method is used. Many "Rife" machines simply do not produce enough power to penetrate all the tissues, which has a major impact on clinical results.

SPECTRUM ANALYSER PATTERN:

- ▶ The carrier frequency and multiple side-band frequencies.
- ▶ **Below:** measured on an original Rife machine.
- ▶ **Right:** measured on the Tru-Rife system.

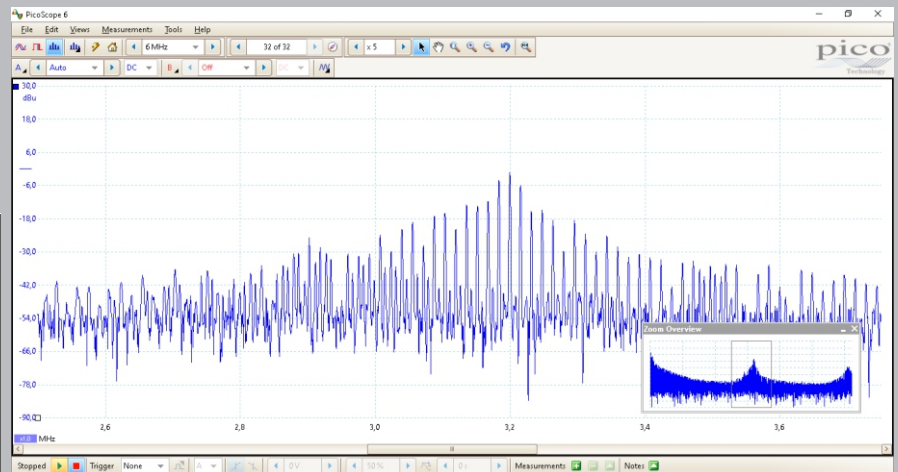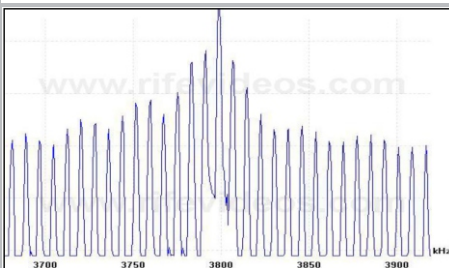

OSCILLOSCOPE PATTERN:

- ▶ The Hoyland wave shape and relative power.
- ▶ **Below:** measured on an original Rife machine.
- ▶ **Right:** measured on the Tru-Rife system.

